



Tray- and drilling protocol guide – Overlay 2

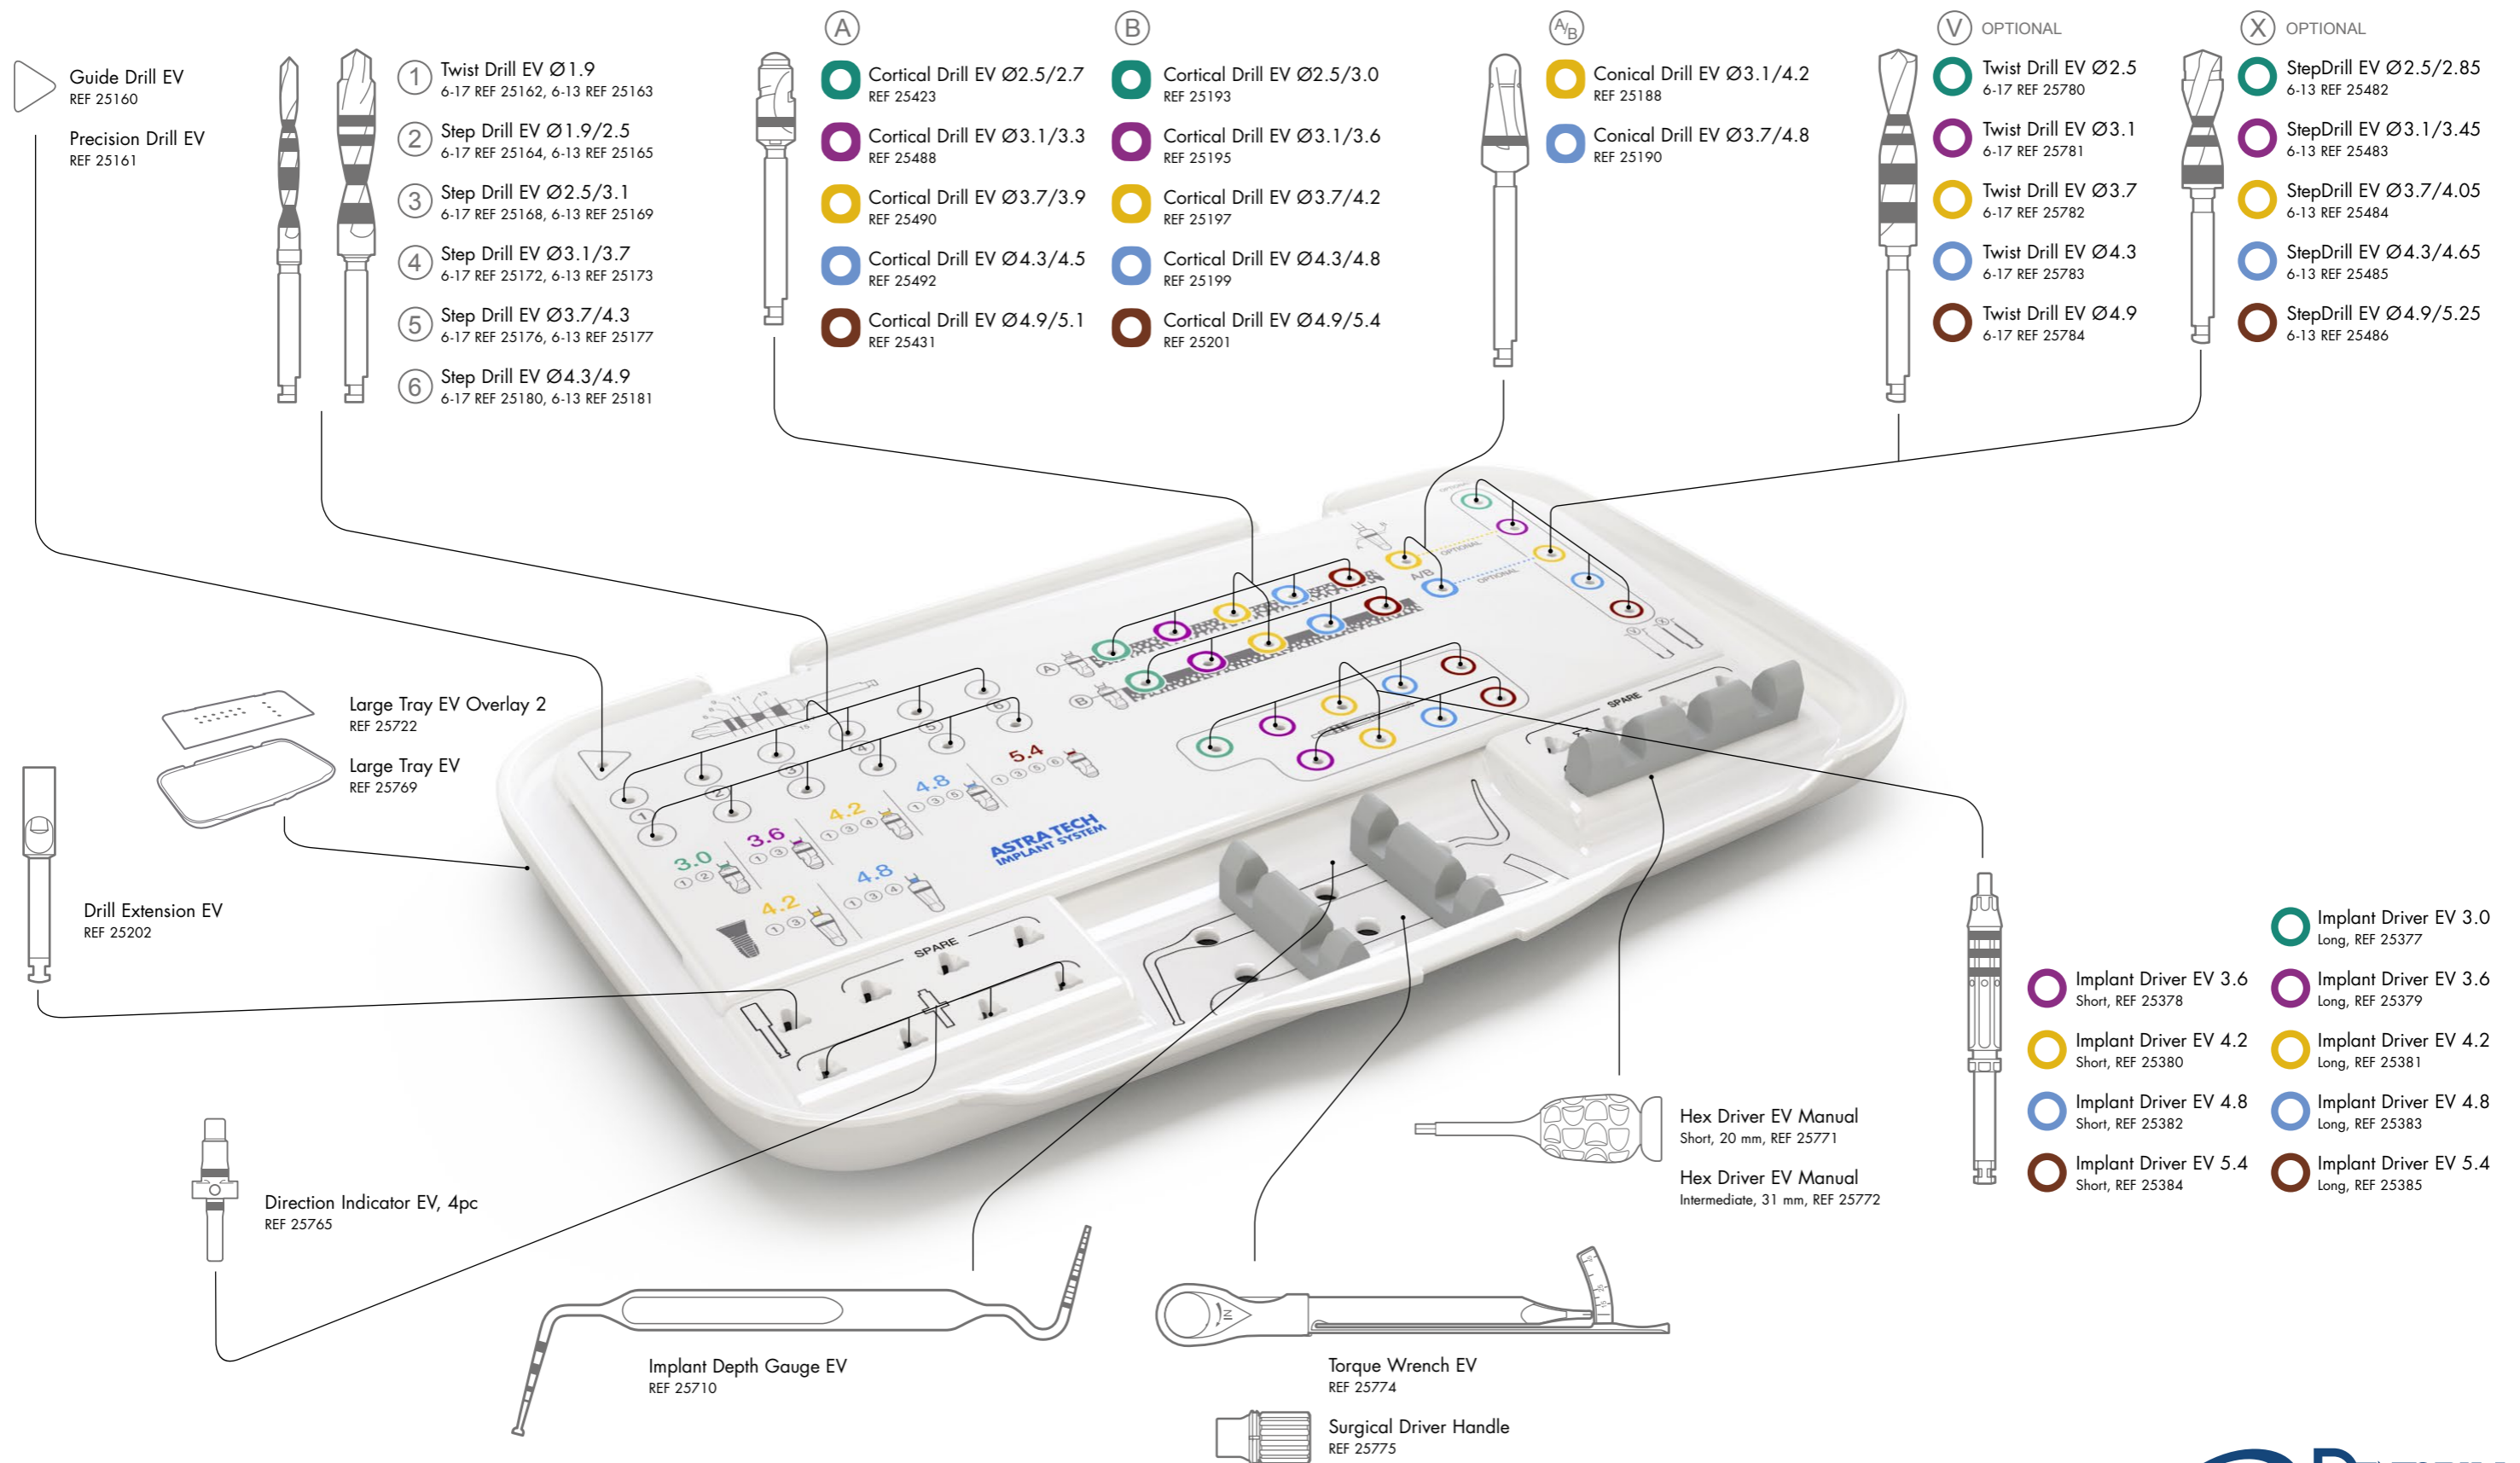

ASTRA TECH IMPLANT SYSTEM

ASTRA TECH Implant System™ EV drilling protocol overview




There is one drilling protocol recommended for preparation of the spongy bone with two options for the cortical bone.

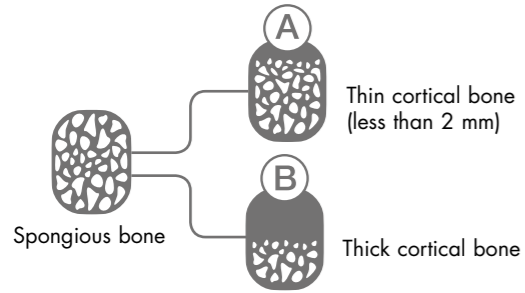

Step Drill


Used for site preparation – allows for a stepped osteotomy that provides guidance during the drilling process.

Length: available in 6–13 mm and 6–17 mm.

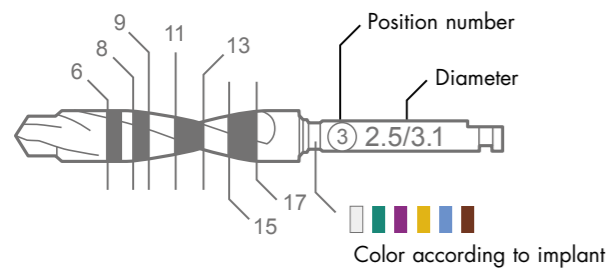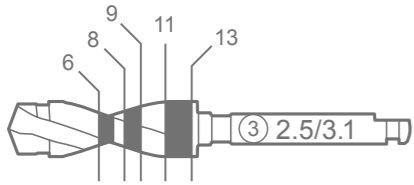



Cortical Drill – straight implants

Used for preparation of the cortical layer.
Note: There are special cortical drills for implants with 6 mm length.




Conical Drill – conical implants

Used for preparation of the cortical layer.
(A) – Thin cortical bone, drill to the apical border of the depth indication line.
(B) – Thick cortical bone, drill to the marginal border of the depth indication line.

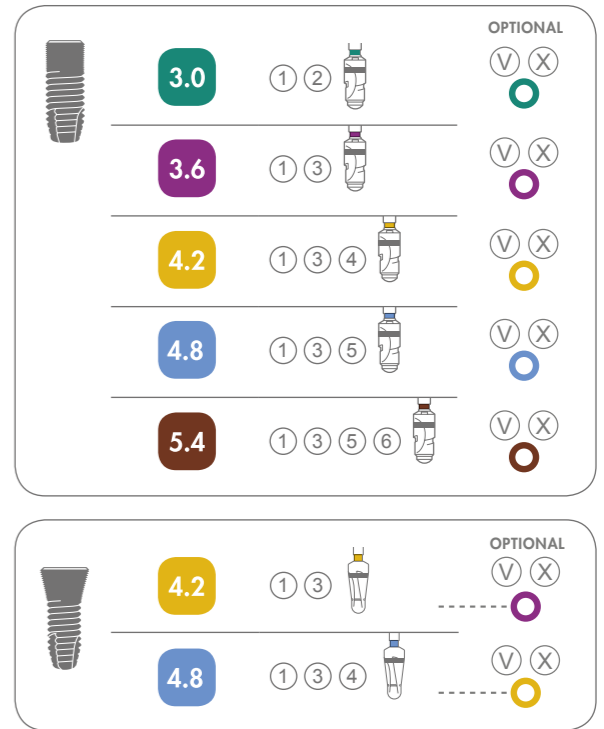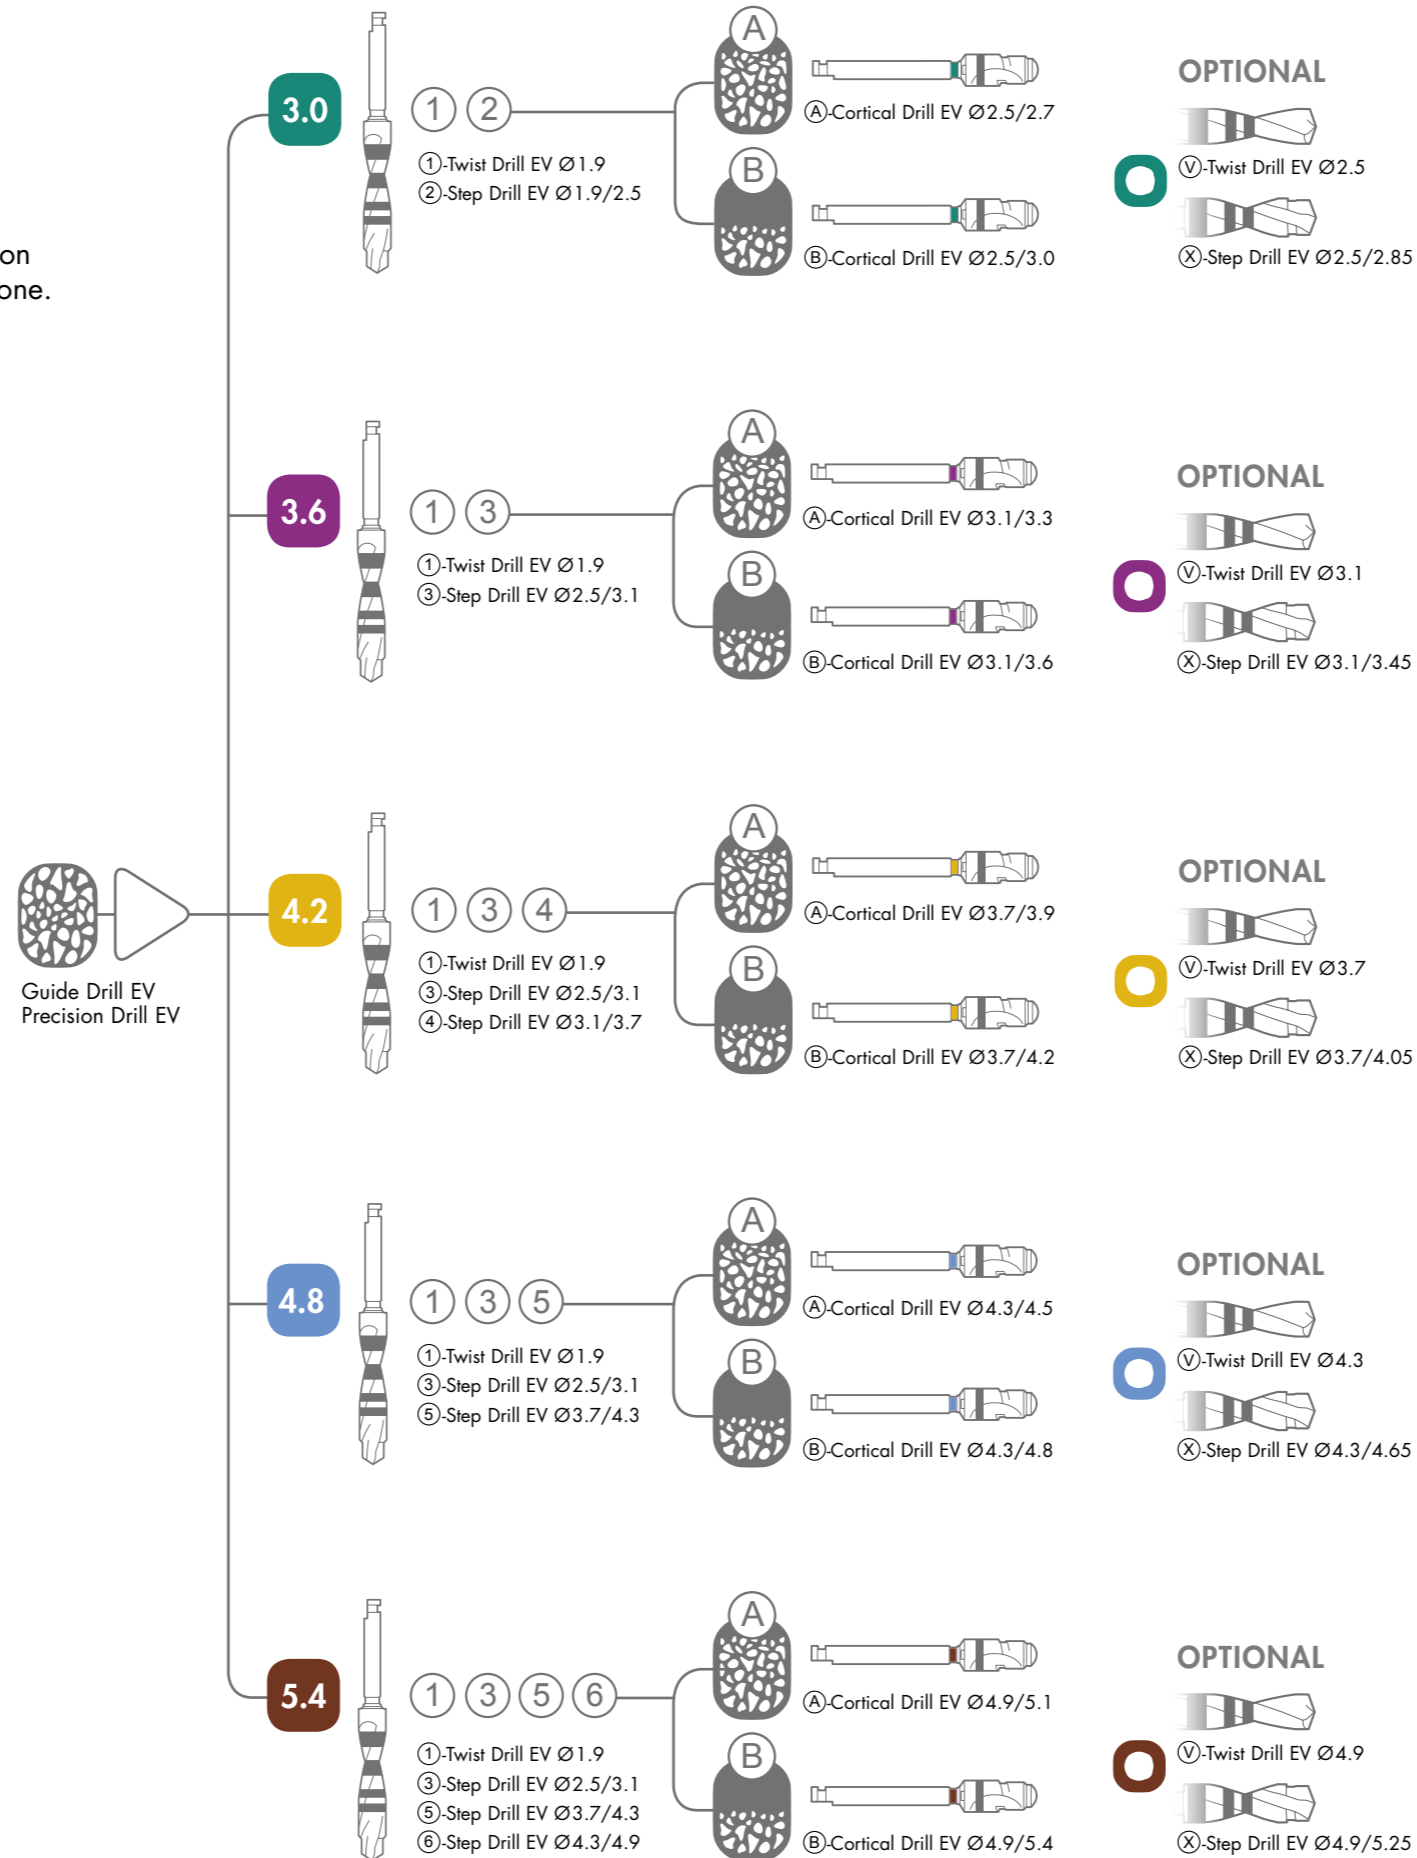

Optional X/V osteotomy preparation

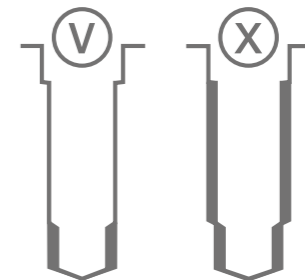

Note: For conical implants, color refers to the diameter of the implant body.